

CALIBRATION CERTIFICATE




Total Weighing Solutions Ltd
 Unit 8 Signal Park, West March
 Daventry, Northants, NN11 4RU, UK
 www.totalweighing.co.uk
 Tel: 01327 368020

Customer Details	
Name:	WHILTON MILL LTD
Address:	WHILTON LOCKS
	DAVENTRY NORTHAMTONSHIRE NN1 2NH
Contact:	DAN
Telephone:	01327 843822

Linearity / Accuracy Test				
Test Point (Kg)	As Found Reading	As Found Deviation	Definitive Reading	Definitive Deviation
0	0.0	0.0	0.0	0.0
60	59.9	-0.1	60.0	0.0
120	119.8	-0.2	120.0	0.0
200	199.7	-0.3	200.0	0.0
300	299.6	-0.4	300.0	0.0

Certificate No.	19283
Date of Calibration:	29/11/2024
Next Due:	29/11/2025

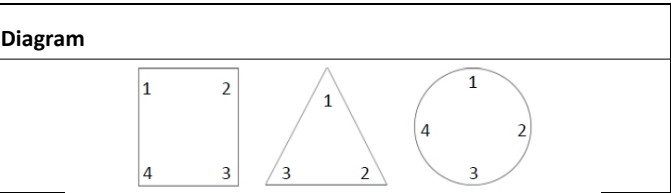

Location:	
Department:	
Manufacturer:	DINI ARGEO
Model:	DFWL B-2
Serial No.:	0722941484
Capacity:	600 Kg
Resolution:	0.1
Tolerance:	+/- 3 divs
Calibration Frequency:	Yearly

Off Centre Load Test				
Test Point (Kg)	As Found Reading	As Found Deviation	Definitive Reading	Definitive Deviation
100.0	100.0	0.0	100.0	0.0
100.0	100.0	0.0	100.0	0.0
100.0	100.0	0.0	100.0	0.0
100.0	100.0	0.0	100.0	0.0

Test Weight/Rig Details
Identification No. and Certificate No.
WEIGHT SET: T1 - T35, D11724 & B12267
CERTIFICATE NUMBER: 12582, 11301, 11303 & 121466
Test weights and equipment are traceable to National Standards

Repeatability Test				
Test Point (Kg)	As Found Reading	As Found Deviation	Definitive Reading	Definitive Deviation
200.0	200.0	0.0	200.0	0.0
200.0	200.0	0.0	200.0	0.0
200.0	200.0	0.0	200.0	0.0

This certificate complies with the United Kingdom Weighing Federation Calibration Code of Practice for non-automatic weighing instruments

Comments	Tolerances
	Unless otherwise agreed, tolerances will be those permitted by current Weights and Measures Regulations for Class III machines as follows:- 0-500 divisions +/- 1div >501-2000 divisions +/- 2div >2001 divisions +/- 3div

Technicians Name Tony Goodman **Technicians Signature**
 Total Weighing Solutions Ltd
 Registered Office: Unit 8 Signal Park, West March, Daventry, Northants, NN11 4RU, UK